


AUXILOCK® KNOTLESS PEEK OPTIMA PUSH-IN SUTURE ANCHOR

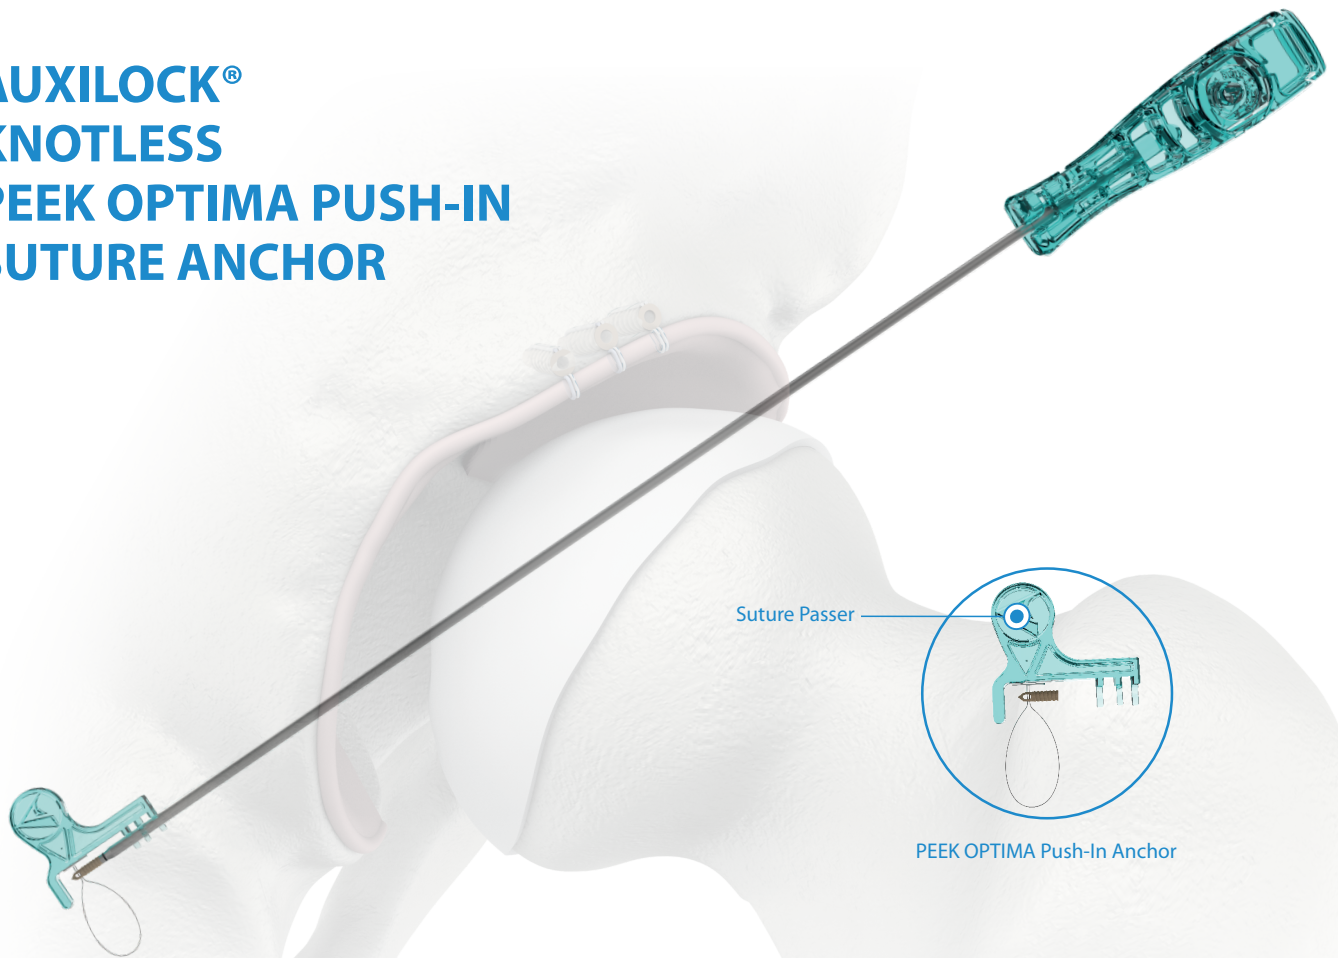

Ordering Information

Code	Product Description
6-039-02	AUXILOCK® 2.8mm Knotless PEEK OPTIMA Push-In Suture Anchor With Hip Length Driver, With Suture Passer (Hip)

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-138-01	8 Point Drill Guide, Long	6-039-02
7-138-02	Ø2.5mm X 360mm Knotless Drill Bit, Long	6-039-02
7-138-03	Trocar Tip Obturator, Long	6-039-02

STERILEEO