


# AUXILOCK® ROTADOR PEEK OPTIMA SCREW-IN ANCHOR

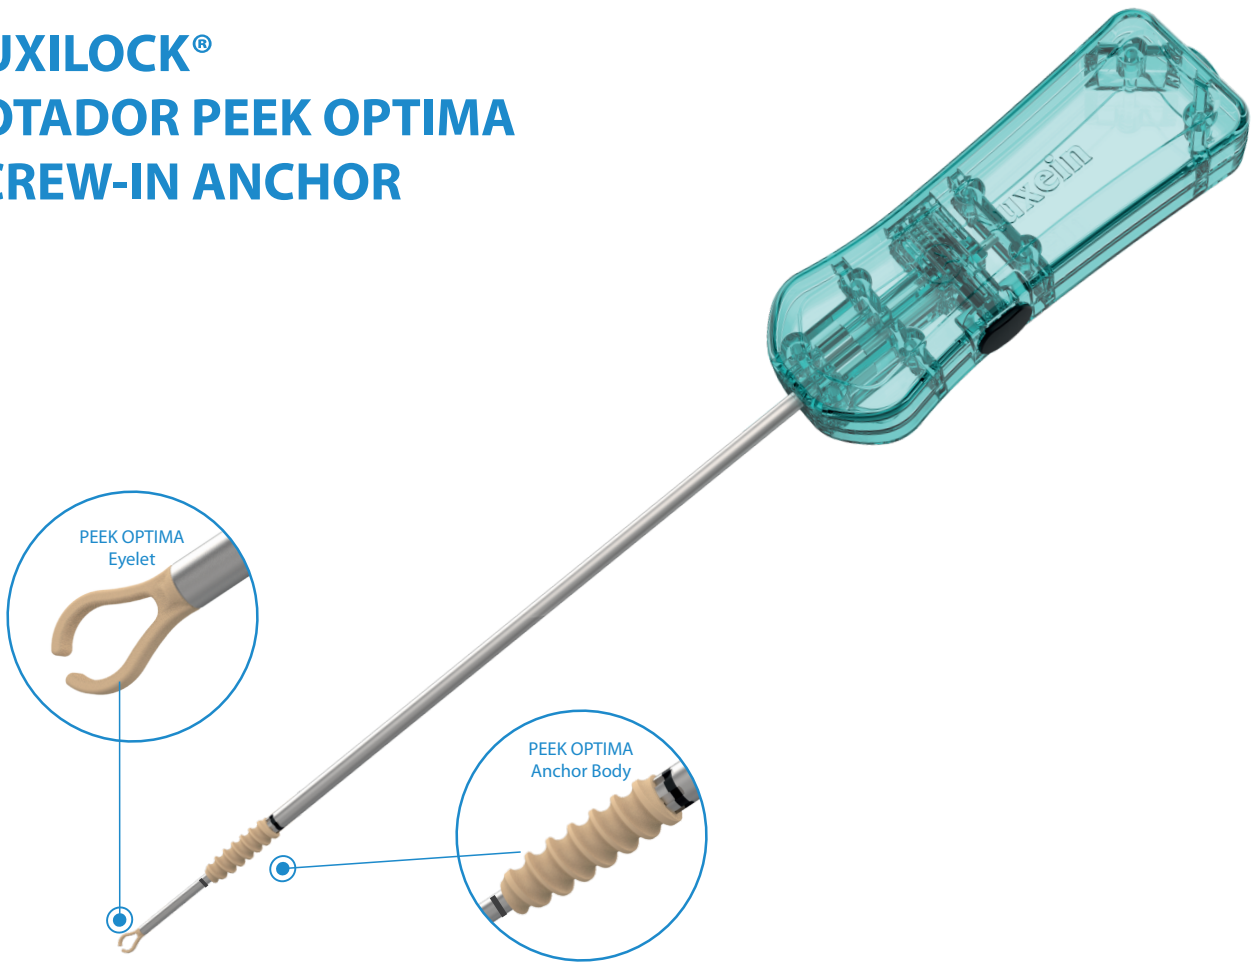

## Ordering Information

Code	Product Description
6-020-01	AUXILOCK® Rotador 4.75mm x 15mm PEEK OPTIMA Screw-In Anchor

## Recommended Instrumentation

Code	Product Description	Compatible Implants
7-139-69	Tap for 4.75 mm Rotador Screw-in Anchor	6-020-01

**STERILE EO**